

# PARAMAGNETIC OXYGEN ANALYZER

DATA SHEET

ZKG

This product is a dumbbell type paramagnetic oxygen analyzer. Because this analyzer is based on that the magnetic susceptibility of oxygen gas is larger than coexisting gases, stable measurement is ensured unaffected by coexisting gases. The detector does not have a heating part such as heater. Therefore, this analyzer is suited for measuring the oxygen concentration in flammable gas. Further, running cost can be saved since reference gas is not required.

## FEATURES

1. Since reference gas is unnecessary due to use of a dumbbell type paramagnetic system, this analyzer will not entail an additional running cost.
2. The principle of measurement is dependent on the strong magnetic property of oxygen molecules. Therefore, measurement is almost unaffected by other molecules weaker in magnetic property than oxygen.
3. Suited for measuring oxygen in flammable gas.
4. Small-sized and easy to handle.
5. Usable with a wide range of power supplies.
6. Output is linear.

## SPECIFICATIONS

### Measuring range:

0 to 10, 21, 25, 50, 100% O<sub>2</sub>

### Number of ranges:

1 or 2 ranges (selectable by code symbol)

### Measuring system:

Paramagnetic (dumbbell type)

### Output signal:

One of the following signals (selectable by code symbol)  
 4 to 20 mA DC (load resistance 550 Ω max.)  
 0 to 1 V DC (permissible load resistance 100 kΩ max.)  
 0 to 10 mV DC (permissible load resistance 100 kΩ max.)

### Repeatability:

Within ±0.5% of full scale

### Linearity:

Within ±1.0% of full scale

### Zero drift:

Within ±2.0% of full scale/week

### Span drift:

Within ±2.0% of full scale/week

### Response time:

Within 15 sec (90% response)

### Flow rate of sample gas:

0.5 L/min ± 0.2 L/min

### Pressure loss:

Approx. 0.3 kPa (at sample gas flow rate 0.5 L/min)



### Flow rate of purge gas (option):

1 L/min, N<sub>2</sub> or air (flowed for purging corrosive ambient gas)

### Power supply:

100 to 240 V AC, 50/60 Hz

### Power consumption:

Approx. 35 VA

### Ambient temperature:

0 to 45°C

### Ambient humidity:

Less than 90% RH

### Warm-up time:

Approx. 30 minutes

### Materials of gas-contacting parts:

SUS304, SUS316, fluororubber, borosilicate glass, Electroless Nickel, platinum, platinum/iridium alloy, PP, Toaron, PVDF (polyvinylidene fluoride), PPS resin

### Interference due to coexisting gas:

Interfering gas	Interfering gas concentration	Interfering concentration
NO	2000ppm	0.15vol% O <sub>2</sub> max.
CO	100vol%	0.1vol%O <sub>2</sub> max.
CO <sub>2</sub>	100vol%	- 0.35vol%O <sub>2</sub> max.
CH <sub>4</sub>	100vol%	- 0.25vol%O <sub>2</sub> max.

### Enclosure:

Steel casing, for indoor application, flush mounting on panel

### Dimensions (H x W x D):

240 x 192 x 234 mm

### Weight:

Approx. 5 kg

### Finish color:

Munsell 10Y7.5/0.5 semi-gloss

**Measuring gas conditions:**

- Temperature: 0 to 50°C
- Humidity: Dew point at least 10°C lower than ambient temperature
- Dust: Max. 100 µg/Nm<sup>3</sup> in particles of max. 0.3 µm each
- Mist: Unallowable
- Pressure: 10 kPa or less


**Installation conditions:**

- The instrument must be protected from direct sunlight and heat radiation from objects at high temperature.
- For installing the instrument outdoors, it must be protected from rain and wind with a suitable casing or cover.
- The instrument must be installed in a clean atmosphere free from corrosive or flammable gas.
- The instrument must be free from severe external vibrations.

**Mounting:**

Vertical mounting on panel


Panel cutout dimensions (mm)



**CODE SYMBOLS**

1 2 3 4 5 6 7 8 9 10		Description
Z	K	Use (4th digit) With indication
G	3	
Y	1	Measuring range (6th digit)
	2	
	3	
	4	
	5	
	0	Purge inlet (7th digit)
	1	
	Y	2nd range (9th digit)
	2	
	3	
	4	
	5	
A		Output signal (10th digit)
B		
C		


**PRINCIPLE OF MEASUREMENT**

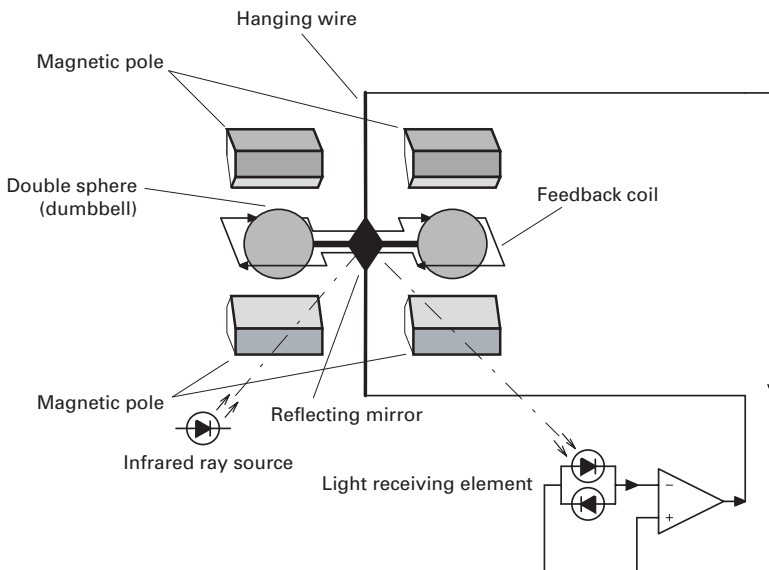

In the cell, two glass spheres filled with nitrogen gas are suspended with strong metal. At first, the spheres are kept in balance in an inhomogeneous magnetic field. When oxygen molecules having a large magnetic susceptibility flow there, the molecules are pulled toward the stronger magnetic field zone and the spheres are moved away from the zone. The resulting deviation of the spheres is detected with the light source, reflecting mirror and light receiving element, and a current is flowed through the feedback loop to control so that the spheres can return to the initial balanced state. The current flowing through the feedback loop is proportional to oxygen concentration. Thus, oxygen concentration is converted into an electric signal.

## CONFIGURATION

### Sampling System Diagram (example: Oxygen measurement in boiler exhaust gas)

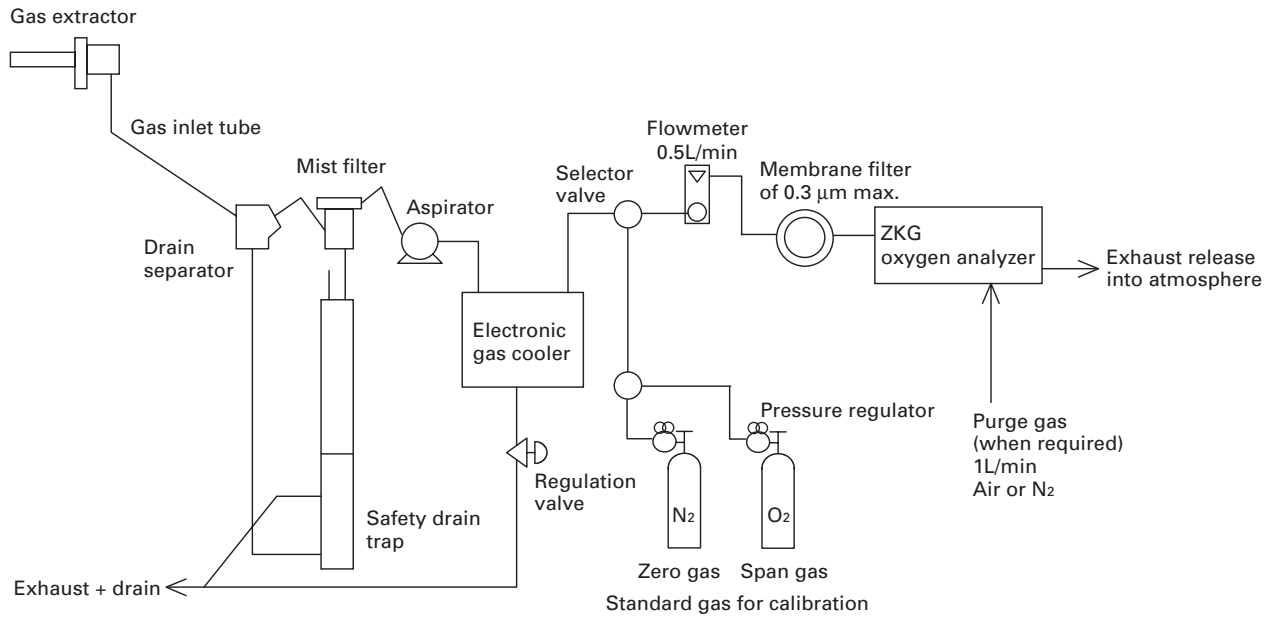



## SCOPE OF DELIVERY

Analyzer main unit x 1  
Panel mounting bracket x 2  
Fuse 250 V AC/0.5 A delay type x 2 (1 accessory and 1 built in)  
Instruction manual x 1

## CAUTIONS



- (1) Use the analyzer within the specified flow rate. If it is used beyond the specified flow rate for enhancing response, the sensor section may be damaged to cause an instrument trouble.
- (2) Before the analyzer, be sure to connect a flowmeter and filter (0.3 μm or finer mesh).
- (3) Use a shielded wire for signal line connection.
- (4) Analyzer exhaust should be released into the atmospheric air.

# OUTLINE DIAGRAM (Unit : mm)

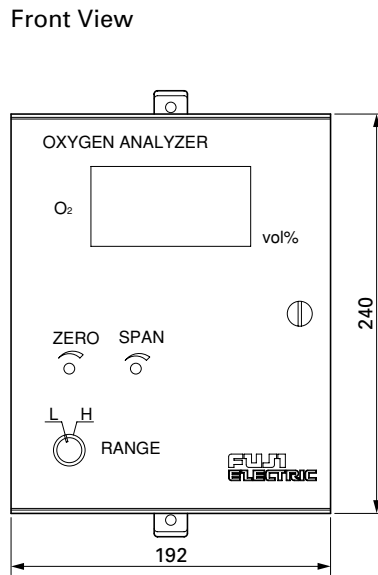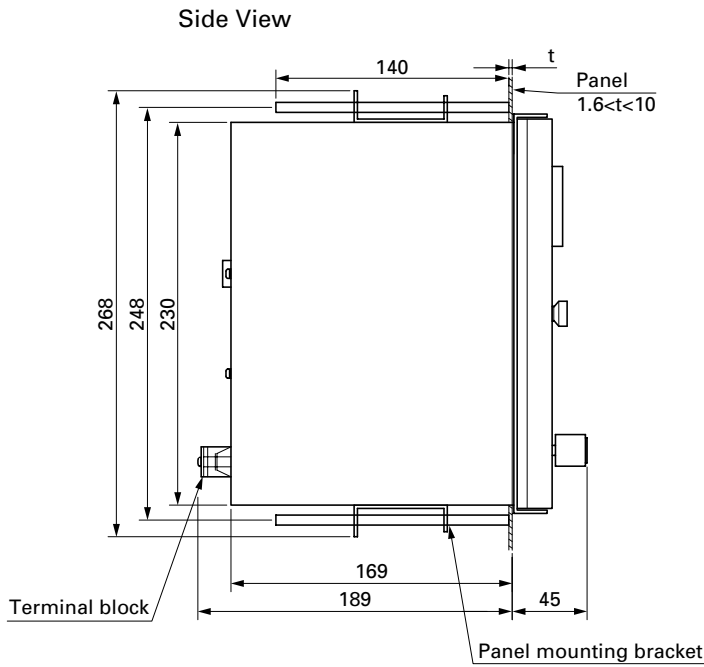


\* Change switch is not attached in the case of a single range.

## PANEL CUTOUT DIMENSION

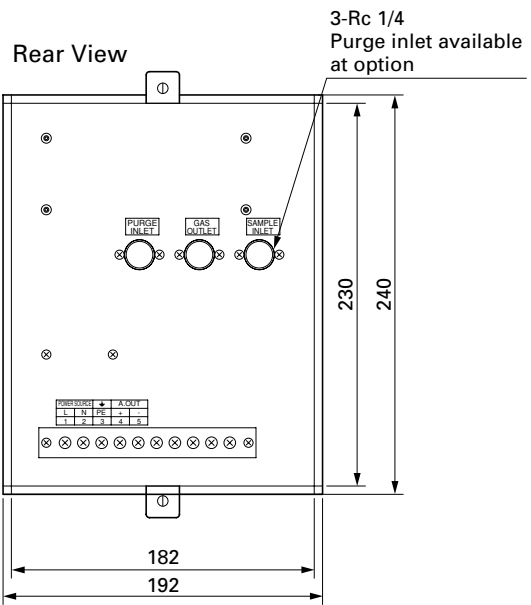

## CONNECTION DIAGRAM

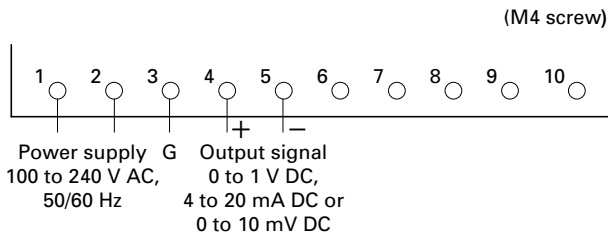

⚠ Caution on Safety

\*Before using this product, be sure to read its instruction manual in advance.

## Fuji Electric Systems Co., Ltd.

### Head Office

Gate City Ohsaki, East Tower, 11-2, Osaki 1-chome,  
Shinagawa-ku, Tokyo 141-0032, Japan  
<http://www.fesys.co.jp/eng>

### Instrumentation Div.

### International Sales Dept.

No.1, Fuji-machi, Hino-city, Tokyo, 191-8502 Japan  
Phone: 81-42-585-6201, 6202 Fax: 81-42-585-6187  
<http://www.fic-net.jp/eng>